



# **Appendix D**

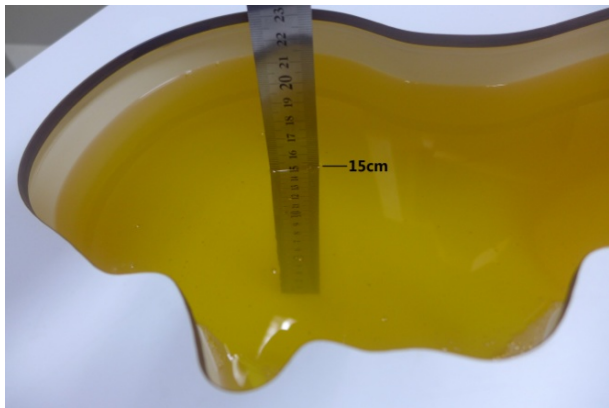
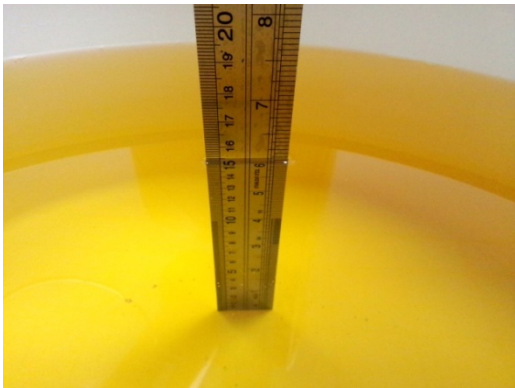
## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details


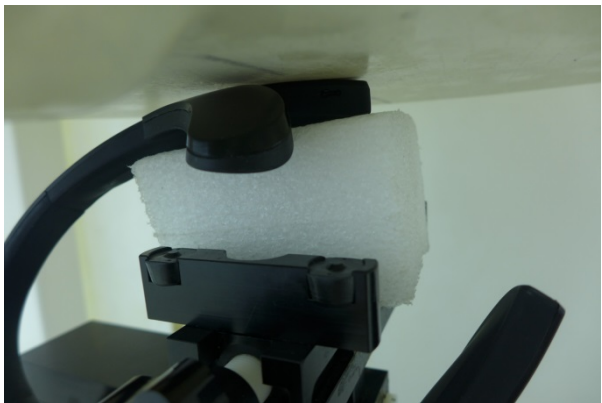

## 1. SAR measurement System



## 2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 2450
 <p>A photograph showing a yellow liquid in a container. A ruler is placed vertically in the liquid, and a label '15cm' points to the liquid level on the ruler.</p>	 <p>A photograph showing a yellow liquid in a container. A ruler is placed vertically in the liquid, and the liquid level is at the 8cm mark on the ruler.</p>

### 3. Photographs of EUT test position

Photo 3: Left touch cheek	Photo 4: Outside 0mm
	
Photo 5: Profile 0mm	NA
	NA

## 4. EUT Constructional Details

